



MP1
spec

ADC

SETUP

Sampl Freq

10 MHz

Amp Ch 1

1 V

Amp Ch 2

1 V

N Points

2048

Pretrigger

0 %

START

ADC Init



STOP

DAC Init



DAC

SETUP

D0 (msec)

50

D4

10

D1

2

D5

5

D8

1

D2

4

D6

1

Phase
Cycling



D3

20

D7

1

File path:

D:\PPG-100\Spectr.pat

N scans

10000

Cur scan

2146

LeftShift

50

RightShift

400

Output datafile

D:\NQR\OUT\Fiduv.out

34000

32000

30000

28000

26000

24000

22000

20000

18000

16000

14000

12000

0

1

2


3

4

Clear

50

0

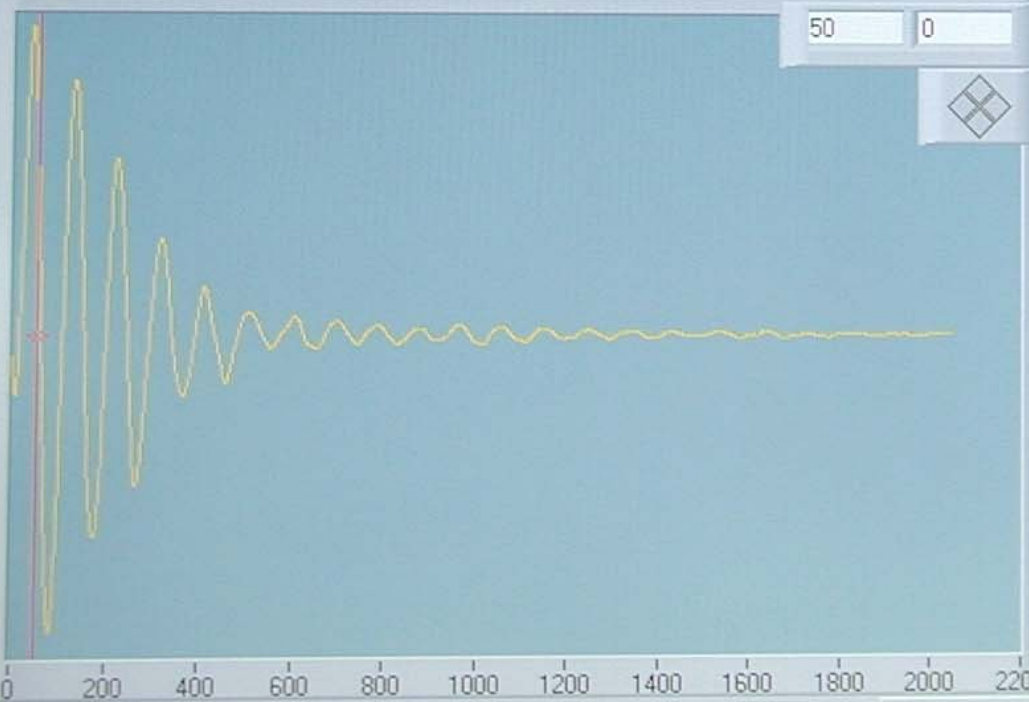

50

0

